

## DEVICE FOR DETECTING ARTERIAL PRESSURE

Technical Field

The present invention relates to a device for detecting arterial pressure. More particularly, the invention relates to a device suitable to  
5 detect arterial pressure, generally known as sphygmomanometer, which is capable of giving maximum objectivity to the measurement made.

Background Art

As is known, the sphygmomanometer was introduced at the end of the 19<sup>th</sup> century and is still universally used today according to the measurement  
10 technique perfected in the early 20<sup>th</sup> century.

Such instrument, composed of a manometer connected to a chamber that can be inflated by means of an air-bulb, is designed to oppose a known pressure to the arterial pressure and therefore allow to read the pressure values when blood flow is detected, by listening with a stethoscope during  
15 decompression of the cuff that contrasts the known pressure, and subsequently, by auscultation, the level at which the action of the cuff no longer affects the detected sounds.

The inflatable chamber, integrated in a cuff that is applied to the arm of the patient, produces on the arm a pneumatic pressure that exceeds the  
20 arterial pressure at a certain point of the compression, interrupting the flow of blood downstream of the cuff. Once the arterial pressure has been exceeded by 20-30 mm Hg, decompression of the cuff is performed by means of a pneumatic valve that is normally integrated in the bulb.

During decompression, the operator listens to the sounds produced by  
25 the artery, detected by means of a stethoscope that is appropriately placed on the arm. In this manner, the operator detects a series of sounds having mutually different tones, intensities and durations, produced by the arterial pulses, which in turn are a consequence of cardiac activity and of the resistance of the arterial vessel. At this point, the operator must determine  
30 which of these pulses represents the systolic value (maximum pressure) and

which one represents the diastolic value (minimum pressure).

The above described measurement of arterial pressure however suffers drawbacks that are due to the fact that the measurement inherently has the following subjective aspects.

- 5           Excessively rapid decompression rate: the error due to an excessively rapid decompression rate in the cuff derives from the reaction time of the operator.

When the operator detects the pulse that determines the systolic value or the one that determines the diastolic value, he/she reads on the graduated  
10 scale of the manometer the value, which in the meantime has decreased as a function of its decompression rate.

As a consequence of this, medical doctrine prescribes a rate between 2 and 3 mm Hg per second as regards decompression. However, in practice this prescription is commonly ignored, because there is a tendency to reduce  
15 the time required for the measurement, underestimating the error made and therefore failing to obtain reliable data.

A second type of error is given by a parallax error, i.e., by an incorrect placement of the operator with respect to the manometer. As is evident, such error can be opposite in sign and variable in meaning, with  
20 random characteristics, indeed depending on the position that the operator assumes with respect to the manometer.

Another error is given by the operator's natural tendency to round off the read value to a value that is easy to memorize. This rounding off is usually performed to 5 mm Hg and sometimes to 10 mm Hg.

- 25           Yet another error is given by the uncertainty in determining which pulse indicates systolic pressure and likewise which pulse indicates diastolic pressure.

In the first case, the phenomenon that causes so-called supermaximal pressure is known in the doctrine. When decompression begins, one waits to  
30 detect the first pulse in the stethoscope. The first pulse normally indicates

the systolic value (maximum pressure). However, the first pulse does not always correspond to flow of blood beneath the inflatable chamber caused by the blood pressure exceeding the pressure that contrasts it by means of the cuff. Actually, with a high-intensity wrist pulse it is possible to detect  
5 pulses produced by the impact of the arterial pulsation against the edge of the cuff that constitutes the obstacle that cannot be passed until its pressure has dropped below the level of the arterial pressure.

Substantially, this noise may be audible with a variable acoustic level depending on the intensity of the wrist pulse. In the presence of a "strong"  
10 pulsation, these supermaximal pulses must be discriminated by the operator by comparing their intensity with the subsequent pulses.

In the second case, there is uncertainty in determining which pulse can be defined as a diastolic pulse, i.e., the pulse that indicates the minimum pressure. Determination of diastolic pressure has always been more difficult  
15 to define, and uniformity of its results is currently unsolved.

Electronic sphygmomanometers are currently known which use the principle of the manual sphygmomanometer but replace auscultation by the operator with detection of the signal by means of a microphone or by detecting the sphygmic pulse in the form of a pneumatic oscillation within  
20 the circuit of the instrument, caused by the arterial pulsation itself.

The first method is the closest possible analogy to stethoscopic auscultation, with the difference of replacing human abilities in hearing and processing the signal with electronic means that can offer different results due to obvious inherent characteristics.

25 The second technique has greater operating differences, since it is not based on the same element described above, i.e., the noise generated by blood flow, but on a different element, such as the pneumatic oscillation inside the circuit of the instrument, caused by the pulsation itself. By processing with increasingly sophisticated algorithms, an attempt has been  
30 made to attain a result that is as close as possible to the result that can be

obtained with human auscultation, but currently it is not possible to have a completely reliable measurement.

#### Disclosure of the Invention

The aim of the present invention is to provide a device for detecting  
5 arterial pressure that substantially allows to improve the precision of the measurement.

Within this aim, an object of the present invention is to provide a device for detecting arterial pressure that allows to eliminate the drawbacks due to an excessively high decompression rate, to parallax error, to the  
10 operator's tendency to round off the measured value, and finally to the uncertainty in determining the pulse to be defined as systolic and the pulse to be defined as diastolic.

A further object of the present invention is to provide a device for detecting arterial pressure that maintains the central role of human  
15 assessment in pressure measurement, supporting it with the aid of electronic means.

A further object of the present invention is to provide a device for detecting arterial pressure that is highly reliable, relatively simple to manufacture, and at competitive costs.

20 This aim and these and other objects that will become better apparent hereinafter are achieved by a device for detecting arterial pressure with high measurement precision, comprising a cuff with inflatable chamber, adapted to be placed around the arm of a patient; means for introducing air to inflate said cuff, and decompression means suitable to decompress said inflatable  
25 chamber, characterized in that it comprises means adapted to detect and store all the sphygmie pulses generated by arterial pressure and to identify the pulses that correspond to the appearance and disappearance of the wrist beat, detected by means of a technique for detecting sphygmie pulses generated by arterial pressure that requires the intervention and judgment of  
30 an operator.

### Brief Description of the Drawing

Further characteristics and advantages of the invention will become better apparent from the description of a preferred but not exclusive embodiment of the device according to the present invention, illustrated by  
5 way of non-limiting example in the accompanying drawing, wherein the only figure is a block diagram of the apparatus according to the present invention.

### Ways of Carrying out the Invention

With reference to the figure, the device according to the present  
10 invention, generally designated by the reference numeral 1, comprises air pumping means 2, for example of the manual or electric type, which are connected to a cuff 3, inside which an inflatable chamber is accommodated. Decompression means 4, conveniently constituted by a compression valve, are adapted to perform a constant and controlled decompression of the cuff  
15 3, as prescribed by medical doctrine to perform an accurate measurement.

The device further comprises means 5 for complete and instantaneous venting of the air of the cuff 3. The venting means 5 are constituted, for example, by a valve that allows to discharge instantly, at the operator's choice, the air from the cuff 3. As an alternative, it is possible to use as a  
20 vent the same decompression valve, used appropriately.

The device according to the invention further has pressure transducer means 6, which are adapted to detect electronically all the sphygmie pulses generated by arterial pulsation and are connected to storage means 7 adapted to store said pulses. The means 6 for detecting the sphygmie pulses  
25 further allow to identify the pulses that correspond to the appearance and disappearance of the pulse, detected by means of any detection method that provides for the intervention of the operator and for his subjective judgment.

The transducer means continuously detect the value of the pressure of  
30 the cuff, like a normal manometer does. This value is reported in real time

by the display and recorded together with the detection of the sphygmic pulses. Accordingly, once the measurement has ended, the operator can analyze, on the display, a listing in which, next to the pressure values expressed for example in mm Hg (or KPa), he/she can read, at the pressure  
5 pulses, a value that indicates their sphygmic intensity.

The operator, when he perceives the stethoscope pulses (or pulses detected in another manner) that correspond to the systolic and diastolic pressure, presses a button of the device to "mark" these values on the digital scale of the device.

10 Substantially, therefore, the user performs a manual detection of the pulses by means of the conventional stethoscope (or, as mentioned, by means of any other method), but the means 6 for detecting sphygmic pulses are associated with said detection and allow to identify the pulses that correspond to systolic pressure and to diastolic pressure.

15 Storage of the data, i.e., of the pulses and therefore of the chart, allows to determine with certainty the pulses that actually correspond to the maximum and minimum values of arterial pressure, performing this analysis after detection by means of the stethoscope.

Substantially, therefore, the operator has control over the  
20 measurements performed manually, and accordingly can associate the precision of manual detection with a device that allows to eliminate the previously mentioned uncertainties that are inherent in the measurement.

The device is further provided with display means 8, which are adapted to display at least the following detected pressure levels: in real  
25 time, at the stored times, with previous measurements (i.e., measurement history).

The device according to the present invention is capable of transferring the detected results to other storage and/or printout means.

It should be noted that the measurement method currently in use, i.e.,  
30 with a cuff provided with an inflatable chamber, prescribes the use of an

inflatable chamber that is proportionate to the size of the arm of the patient. However, since in practice it is not possible to have a cuff for each patient, medical doctrine has established three types of cuffs for three different types of patient. However, very often an operator does not comply with these  
5 indicators and always uses a single standard cuff.

The use of a standard cuff, however, is another source of error, which adds to the previously described errors that are inherent in the measurement.

For this purpose, the device according to the present invention uses a cuff 3 on which a scale is printed along its entire longitudinal side, said  
10 scale indicating, when the cuff is applied, the circumference of the arm of the user. This information can be used, by entering it in the device according to the invention, as a corrective factor for the arterial pressure measurement that is made, accordingly complying with the criteria of using a cuff for each type of patient.

15 In practice it has been found that the device according to the present invention allows to perform a manual measurement with a stethoscope of the arterial pressure of a patient, with the association of means adapted to detect the sphygmie pulses generated by arterial pressure and to then identify the pulses that correspond to the appearance and disappearance of  
20 the pulse detected by means of the stethoscopic technique. These pulses correspond respectively to systolic pressure and to diastolic pressure.

The operator, therefore, can perform a manual measurement with the aid of a sort of electronic measurement for control and confirmation. The device according to the invention allows to store the chart of the pulses in  
25 order to perform a subsequent verification thereof, so as to determine assuredly the pulses that actually correspond to the maximum and minimum values of the arterial pressure.

The device thus conceived is susceptible of numerous modifications and variations, within the scope of the appended claims. All the details may  
30 be replaced with other technically equivalent elements.

In practice, the materials used, as well as the contingent shapes and dimensions, may be any according to requirements and to the state of the art.

The disclosures in Italian Patent Application No. MI2003A001683 from  
5 which this application claims priority are incorporated herein by reference.



CLAIMS

1. A device for detecting arterial pressure with high measurement precision, comprising a cuff with inflatable chamber, adapted to be placed around the arm of a patient, means for introducing air to inflate said cuff,  
5 and decompression means adapted to decompress said inflatable chamber, characterized in that it comprises means adapted to detect and store all the sphygmie pulses generated by the arterial pulsation and to identify the pulses that correspond to the appearance and disappearance of the wrist beat, detected by means of a technique for detecting sphygmie pulses  
10 generated by arterial pressure that provides for the intervention and subjective judgment of an operator.

2. The device according to claim 1, characterized in that said decompression means of said inflatable chamber comprise a valve for providing constant and time-controlled decompression.

15 3. The device according to claim 1, characterized in that it comprises discharge means adapted to completely and instantaneously discharge the inflatable chamber of said cuff.

4. The device according to one or more of the preceding claims, characterized in that said means for detecting and storing the sphygmie  
20 pulses are connected to data storage means, which are adapted to store the chart of the sphygmie pulses.

5. The device according to one or more of the preceding claims, characterized in that it comprises a display that is adapted to display the detected levels of pressure and the levels of sphygmie intensity of the  
25 pulsations.

6. The device according to one or more of the preceding claims, characterized in that it comprises a button that is adapted to be pressed by the operator when the operator detects sphygmie pulses that correspond to the systolic or diastolic pressure.

30 7. A method for detecting arterial pressure, comprising the steps of:

pumping air into a cuff provided with an inflatable chamber;  
decompressing said inflatable chamber;

detecting, by means of the intervention and subjective judgment of an operator, the sphygmie pulses that correspond respectively to the  
5 appearance and disappearance of the wrist beat,

characterized in that it comprises the steps of:

detecting and storing all the sphygmie pulses generated by arterial pulsation by using an electronic sensing and storage circuit;

identifying, among said sphygmie pulses, the ones that correspond to  
10 the appearance and disappearance of the pulse beat, detected by means of said stethoscope.

8. The method according to claim 7, characterized in that said step of performing the decompression of said inflatable chamber comprises the execution of decompression at a controlled and constant rate.

15 9. The method according to one or more of claims 7 and 8, characterized in that it comprises a step of storing said sphygmie pulses generated by arterial pulsation, in order to allow subsequent analysis of the chart of sphygmie pulses, in order to determine assuredly the pulses that actually correspond to the maximum and minimum values of arterial  
20 pressure.

10. The method according to claim 7, characterized in that it comprises a step of pressing, on the part of said operator, a button when sphygmie pulses that correspond to systolic and diastolic pressure are detected, said sphygmie pulses that correspond to systolic and diastolic  
25 pressure being "marked" on a digital scale of said device.

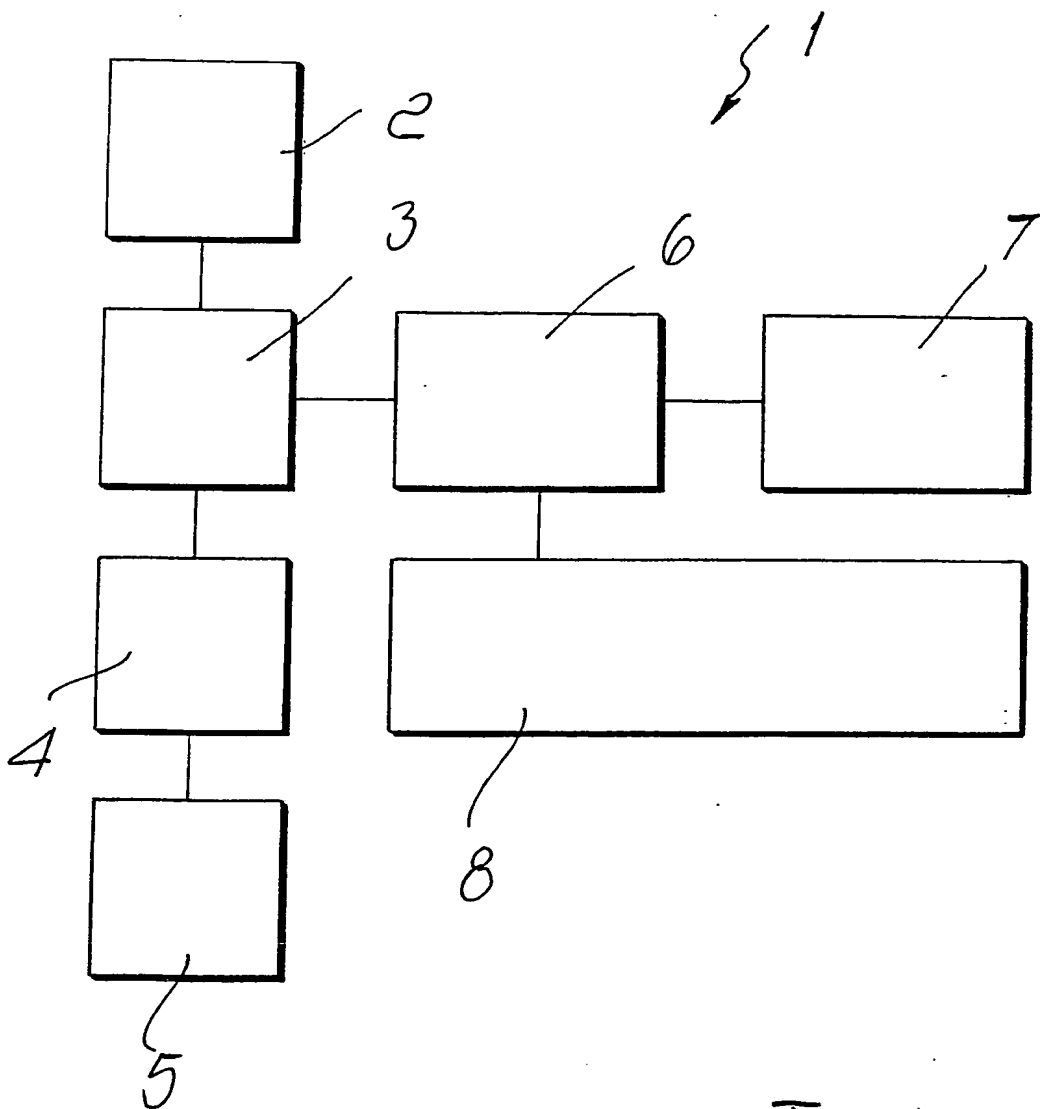


Fig. 1

**THIS PAGE BLANK (USPTO)**

# INTERNATIONAL SEARCH REPORT

International Application No  
PCT/EP2004/009433

A. CLASSIFICATION OF SUBJECT MATTER  
IPC 7 A61B5/0285 A61B5/022 A61B5/024

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)  
IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the International search (name of data base and, where practical, search terms used)

EPO-Internal

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 0 472 464 A (SONY CORP) 26 February 1992 (1992-02-26) column 1 - column 4; figures 2,3	1-10
X	EP 0 506 520 A (SONY CORP) 30 September 1992 (1992-09-30) column 1 - column 3; figures 1-3	1-10

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

### \* Special categories of cited documents:

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

- \*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- \*&\* document member of the same patent family

Date of the actual completion of the international search

17 December 2004

Date of mailing of the international search report

27/12/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Gaillard, A

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/EP2004/009433

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 0472464	A	26-02-1992	JP 6197872 A	19-07-1994
			DE 69115599 D1	01-02-1996
			DE 69115599 T2	02-05-1996
			EP 0472464 A1	26-02-1992
			KR 167776 B1	01-05-1999
			US 5249467 A	05-10-1993
EP 0506520	A	30-09-1992	JP 3006123 B2	07-02-2000
			JP 4288131 A	13-10-1992
			DE 69221654 D1	25-09-1997
			DE 69221654 T2	29-01-1998
			EP 0506520 A2	30-09-1992
			KR 190943 B1	15-06-1999
			US 5396895 A	14-03-1995
			US 5365930 A	22-11-1994